


Tray layout card – T2 Alpha Femur Antegrade Distal Targeting Tray

IMN Instruments System

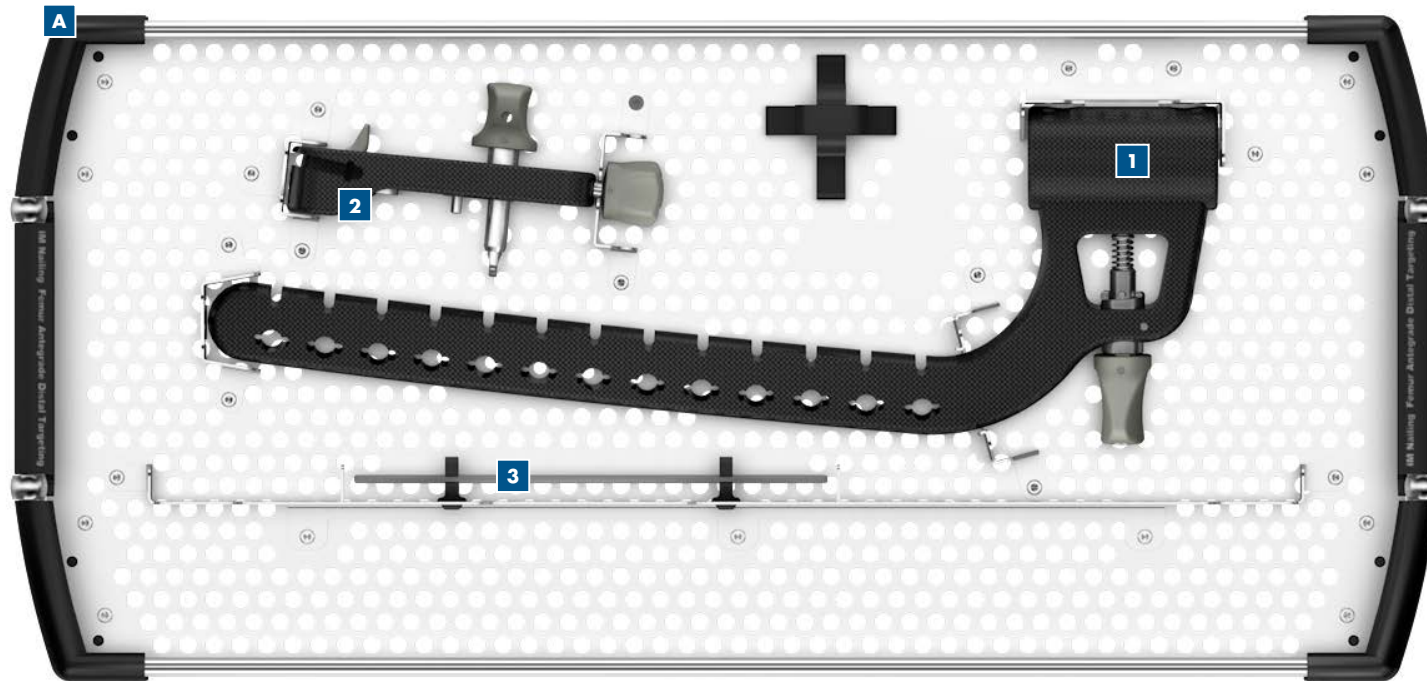

	Ref #	Description	Qty.
A	2355-3050	Femur Antegrade Distal Targeting Tray	
1	2353-3106	Distal Targeting Arm Femur Antegrade	1
2	2353-3105	Adjusting Device Femur Antegrade	1
Optional			
3	1320-5395	Oblique Alignment Wire	2

A surgeon must always rely on his or her own professional clinical judgment when deciding whether to use a particular product when treating a particular patient. Stryker does not dispense medical advice and recommends that surgeons be trained in the use of any particular product before using it in surgery.

The information presented is intended to demonstrate the breadth of Stryker product offerings. A surgeon must always refer to the package insert, product label and/or instructions for use before using any Stryker product. Products may not be available in all markets because product availability is subject to the regulatory and/or medical practices in individual markets. Please contact your Stryker representative if you have questions about the availability of Stryker products in your area. Stryker Corporation or its divisions or other corporate affiliated entities own, use or have applied for the following trademarks or service marks: Stryker, T2 Alpha. All other trademarks are trademarks of their respective owners or holders.

Content ID: T2-TLC-1, 08-2018
Copyright © 2018 Stryker

Stryker Australia
8 Herbert Street,
St Leonards NSW 2065
T: 61 2 9467 1000
F: 61 2 9467 1010

Stryker New Zealand
PO Box 17-136
Greenlane Auckland 1546
T: 64 9 573 1890
F: 64 9 573 1891

stryker.com