


Biofoam[®]

Wedge system

Innovative Cancellous Titanium™ provides consistent strength and fixation for osteotomies.

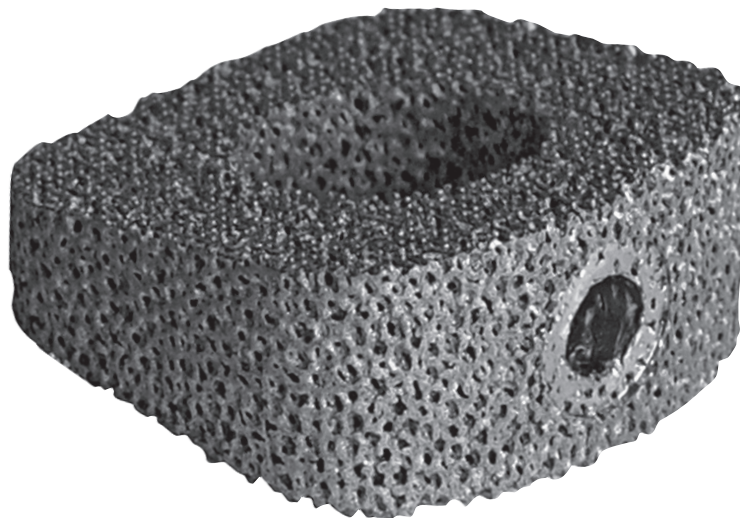

Innovative Cancellous Titanium provides consistent strength and fixation for osteotomies.

Maintained strength

Biofoam Cancellous Titanium matrix maintains its compressive strength throughout the remodeling process.*

Designed for precise and reliable correction

Wedges available in two orientations and 15 sizes designed to provide reliable and precise correction.

Sustainable rigid fixation


High coefficient of friction allows for a stable environment for integration.*

Extensive bone ingrowth

Porosity of the osteoconductive matrix allows for integration of bone.*

Specific, sterile design

Ingrowth potential with low risk of an immune response sometimes related to traditional allografts.*

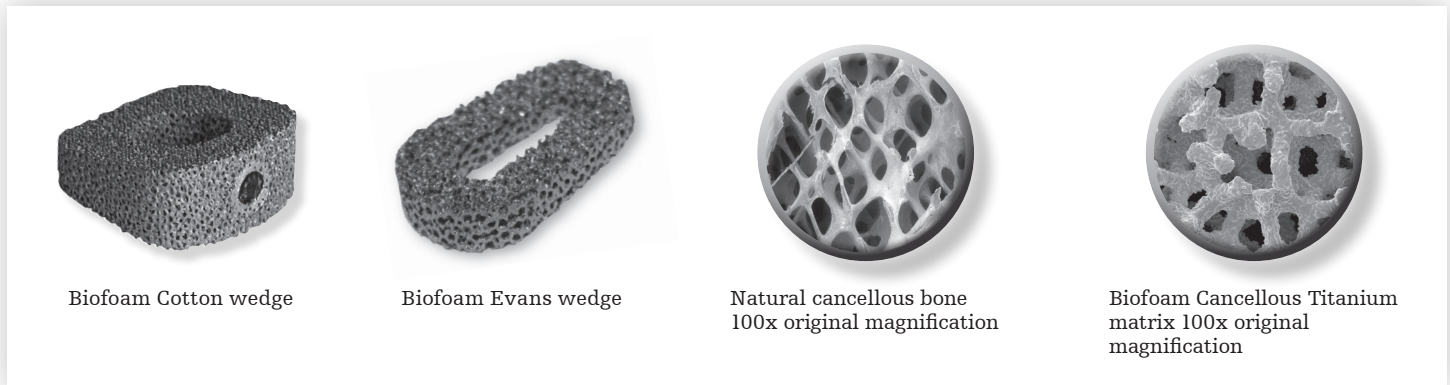

*Data on file

More information

- Biofoam wedge system operative technique 009157A

Alternative products

- Allopure[®] wedges
- Darco[®] PIA plate

Complementary products

- Charlotte[®] Claw[®] plates
- Charlotte compression staple
- Allomatrix[®] DR graft



Allopure wedges



Charlotte 4-hole Claw plate



Charlotte staples

Foot & Ankle

This document is intended solely for the use of healthcare professionals. A surgeon must always rely on his or her own professional clinical judgment when deciding whether to use a particular product when treating a particular patient. Stryker does not dispense medical advice and recommends that surgeons be trained in the use of any particular product before using it in surgery.

The information presented is intended to demonstrate a Stryker product. A surgeon must always refer to the package insert, product label and/or instructions for use, including the instructions for cleaning and sterilization (if applicable), before using any Stryker product. Products may not be available in all markets because product availability is subject to the regulatory and/or medical practices in individual markets. Please contact your Stryker representative if you have questions about the availability of Stryker products in your area. Stryker Corporation or its divisions or other corporate affiliated entities own, use or have applied for the following trademarks or service marks: Salvation, Velcro, Stryker. All other trademarks are trademarks of their respective owners or holders.

AP-015564, 19-Oct-2021

Copyright © 2021 Stryker



Manufactured by:
Wright Medical
Technology, Inc.
1023 Cherry Road
Memphis, TN 38117

stryker.com