

Strength & Flexibility

In Soft-Tissue Repair

PEEK IntraLine Anchor



PEEK IntraLine

Suture Anchor

PEEK IntraLine Anchor

The PEEK IntraLine is a fully-threaded anchor with a suture eyelet. The Force Fiber suture eyelet runs through the center of the anchor, providing flexibility for the working suture.

Offered in 5.5mm and 6.5mm sizes, with and without needles, the PEEK IntraLine Anchor is an excellent tool for rotator cuff and other soft-tissue repairs.

Features:

Suture eyelet.


Fully threaded anchor design.

5.5mm and 6.5mm sizes.

With and without needles.

Simple Handle Design for Open Cases

The PEEK IntraLine Anchor is excellent for arthroscopic and open cases. For open cases, the needles are loaded on Force Fiber Suture and housed in the handle. Once the anchor is implanted, simply slide open the handle and remove the needles. The distal end of the shaft on the version with needles is slotted for simplicity and ease of use.

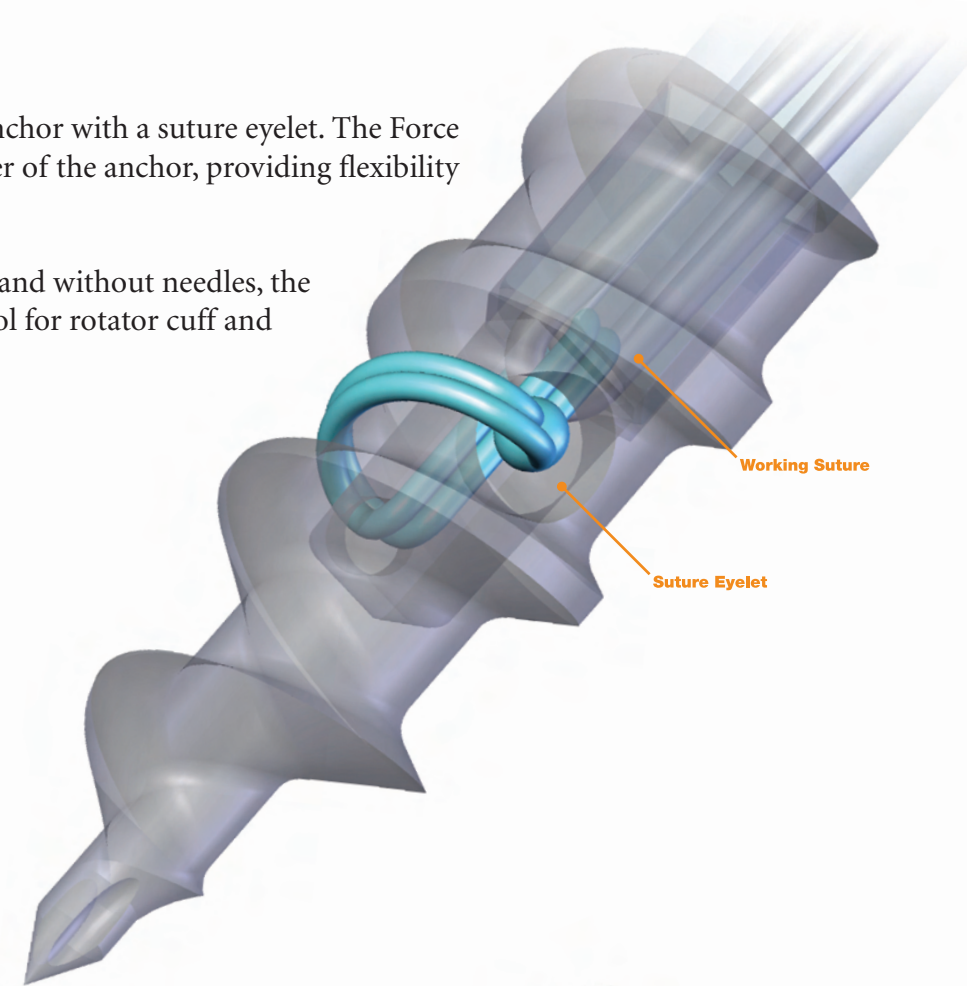

Strength & Flexibility

In Soft-Tissue Repair

PEEK IntraLine Anchor

For arthroscopic repairs, the PEEK IntraLine Anchor features a fully cannulated shaft to house the high-strength Force Fiber working suture. The handle is large for better grip and ergonomics. At the proximal end of the handle, the suture is neatly wound. With one straight pull, the suture simply unwinds and the inserter is ready to be removed. The PEEK IntraLine Anchor is designed for a quick and simple delivery.



Punch-Tap Features:

Punch and tap with one instrument.

Optimized for use with 5.5mm and 6.5mm PEEK IntraLine anchors.

Available in 5.5mm and 6.5mm sizes.





Joint Replacements

Trauma, Extremities & Deformities

Craniomaxillofacial

Spine

Biologics

Surgical Products

Neuro & ENT

Interventional Pain

Navigation

Endoscopy

Communications

Imaging

Patient Handling Equipment

EMS Equipment

325 Corporate Drive
Mahwah, NJ 07430
t: 201 831 5000

www.stryker.com

A surgeon should always rely on his or her own professional clinical judgment when deciding to use which products and/or techniques on individual patients. Stryker is not dispensing medical advice and recommends that surgeons be trained in orthopaedic surgeries before performing any surgeries.

The information presented is intended to demonstrate the breadth of Stryker product offerings. Always refer to the package insert, product label and/or user instructions before using any Stryker product. Products may not be available in all markets. Product availability is subject to the regulatory or medical practices that govern individual markets. Please contact your Stryker representative if you have questions about the availability of Stryker products in your area.

Stryker Corporation or its divisions or other corporate affiliated entities own, use or have applied for the following trademarks or service marks: PEEK, IntraLine, Stryker. All other trademarks are trademarks of their respective owners or holders.

Literature Number: 1000-900-577A Rev. 1
MS/GS 05/08

Copyright © 2008 Stryker
Printed in USA