


Tray layout card – T2 Alpha Basic Instruments Tray


IMN Instruments System

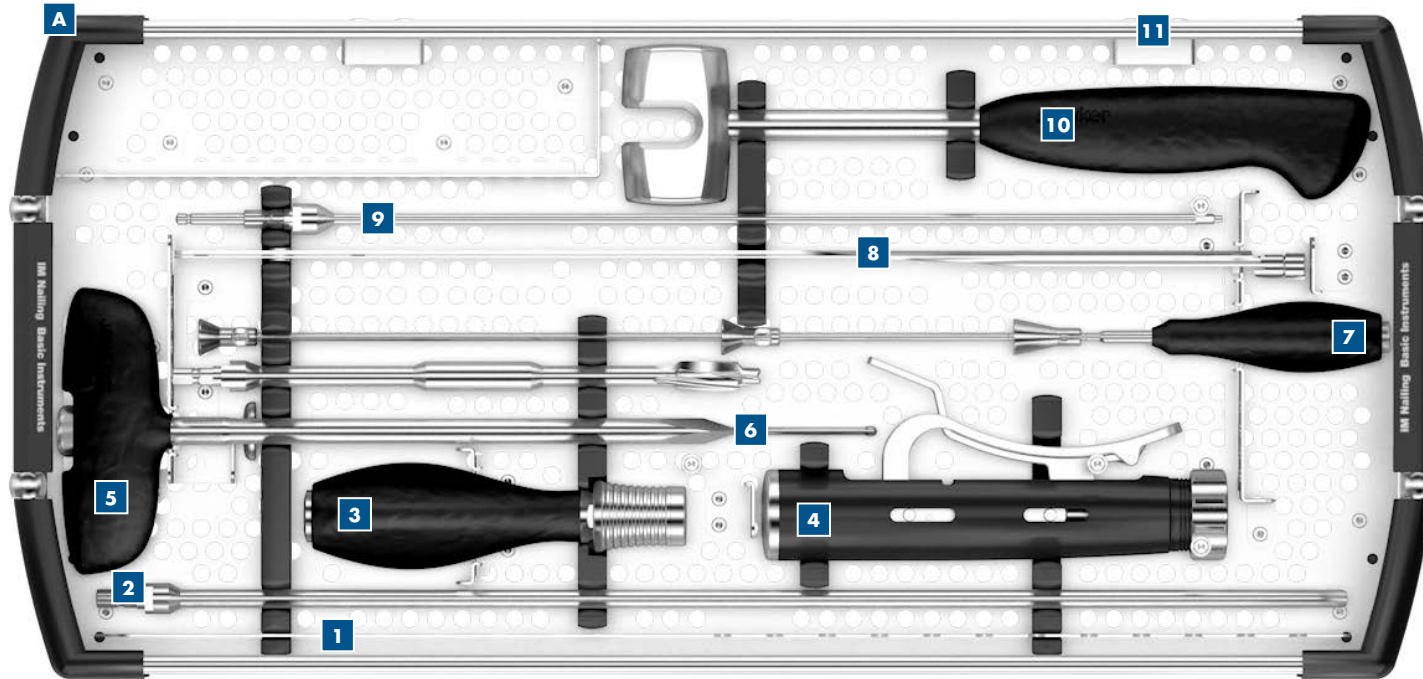

Ref #	Description	Qty.	Ref #	Description	Qty.
A 2355-5000	Basic Instruments tray		6 2351-0011	Awl Plug	1
1 2351-0420	X-ray Ruler	1	7 2351-0380	Guide Wire Pusher	1
2 2351-0020	Reduction Rod	1	8 1806-0022	Guide Wire Ruler	1
3 2351-0140	Quick-Lock Delta Handle, Modified Trinkle	1	9 2351-0400	Compression Screwdriver	1
4 2351-0030	Guide Wire Handle	1	10 2351-0060	Slotted Hammer	1
5 2351-0010	Curved Awl	1	11 2351-5005	Basic Tray Base	1

Tray layout card – T2 Alpha Basic Instruments Tray

IMN Instruments System

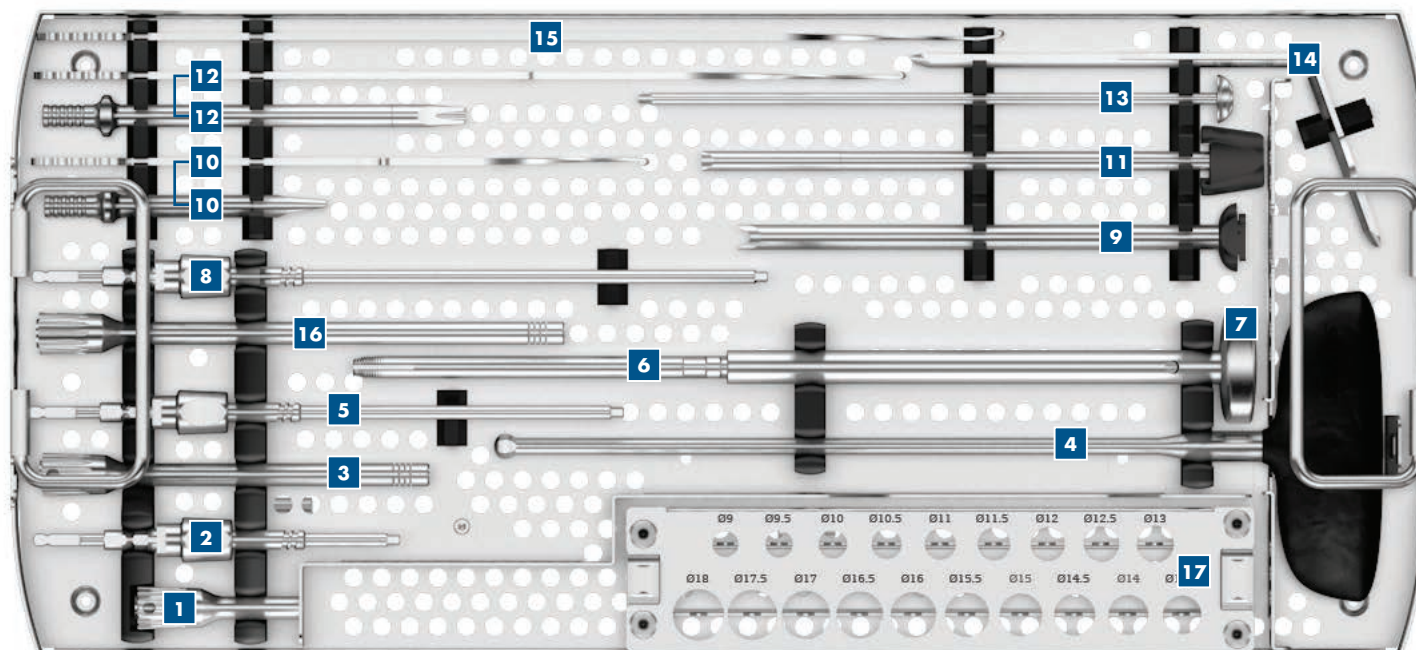

Ref #	Description	Qty.	Ref #	Description	Qty.	Ref #	Description	Qty.
1	2351-0101 Self-Retaining Screwdriver Sleeve, Short	1	7	2351-0050 Delta Strike Plate	1	14	2351-0340 Screw Scale	1
2	2351-0100 Screwdriver Bit, Short	1	8	2351-0110 Screwdriver Bit, Long	1	15	2351-0150 Guided Depth Gauge	1
3	2351-0105 Screwdriver Bit, Medium	1	9	2351-0070 Tissue Protection Sleeve, Long	1		2355-5010 Basic Tray Insert	1
4	2351-0040 Ball Tip Screwdriver	1	10	2351-0160 Freehand Depth Gauge, Short	1	Optional		
5	2351-0106 Self-Retaining Screwdriver Sleeve, Medium	1	11	2351-4280 Locking Drill Sleeve, Long	1	16	2351-0111 Self-Retaining Screwdriver Sleeve, Long	1
6	2351-0180 Extraction Shaft	1	12	2351-0170 Freehand Depth Gauge Long	1	17	2351-0370 Reamer Head Insert	1
			13	2351-4290 Locking Trocar, Long	1			

A surgeon must always rely on his or her own professional clinical judgment when deciding whether to use a particular product when treating a particular patient. Stryker does not dispense medical advice and recommends that surgeons be trained in the use of any particular product before using it in surgery.

The information presented is intended to demonstrate the breadth of Stryker product offerings. A surgeon must always refer to the package insert, product label and/or instructions for use before using any Stryker product. Products may not be available in all markets because product availability is subject to the regulatory and/or medical practices in individual markets. Please contact your Stryker representative if you have questions about the availability of Stryker products in your area. Stryker Corporation or its divisions or other corporate affiliated entities own, use or have applied for the following trademarks or service marks: Stryker, T2 Alpha. All other trademarks are trademarks of their respective owners or holders.

Content ID: T2-TLC-3, 09-2018
Copyright © 2018 Stryker



Manufacturer:
Stryker Trauma GmbH
Prof.-Küntschers-Str. 1-5
24232 Schönkirchen
Germany

stryker.com